

Size Information

Size	S	M	L	XL	XXL
CM	30-34	34-38	38-42	42-46	46-50

Knee Brace

Knee Sizing Guide-Measure around knee joint



Washing Instruction

Washing in cold water, gentle cycle and a mild soap.
Do not dry clean or tumble dry.
Do not use bleach.
Dry in an air current, and do not expose this brace to any heat source.

Caution

Do not wear e-life supports if longterm covering cause allergic reactions please consult your physicians.
Do not use more than 24 hours of continuous.

Indication

Patellar tendinopathy
Osgood-Schlatter disease
Jumper's knee

Contraindication

- Paraesthesia
- Severe varicose vein
- Skin disorders or injuries in the relevant area
- Impaired lymphatic drainage

Recommendation

These products are to be used only by those which have been medical specialist. In order to dispose of the product, comply with the legal norms of your country. If any serious incident that has occurred in relation to the device should be reported to the manufacturer and the competent authority of the Member State in which the user and/or patient is established.

Classification

Class I medical device, non sterile, no measurement function. This product fulfils the Medical Device Regulation (EU) 2017/745.

Manufactured By:

e-life International Co., Ltd.

Head Office:

7F, No.1, Baosheng Rd., Yonghe Dist., New Taipei City 234, Taiwan (R.O.C.)

Tel: +886-2-29231516

Fax: +886-2-29290783

E-mail: info@e-lifebracing.com

www.e-lifebracing.com

Made in Taiwan



e-life

Application Instruction


Q-Fit PATELLAR STRAP




2020 version 1

INSTRUCTIONS FOR USE


E-KNR005 Q-Fit PATELLAR STRAP




1. Measure circumference of knee joint.
2. Refer to sizing chart to select proper size.




5. Then the back strap goes around the back of knee and close the buckle.



3. Pull up the reel and release the lace and detach the buckle.




6. Ensure the the back strap covers two sides of front strap evenly.
7. Then press down the reel and clockwise turn. If too tight, just reversely turn to micro releasing lace.




4. Place the tube on the patellar tendon first (Note : the reel side should be at lateral side; buckle side should be at medial side.)

How to use closure system?

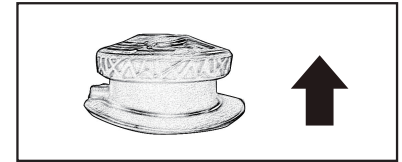

1. Pull up the reel to release the lace

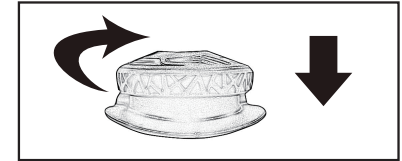

2. Press the reel down and then clockwise turn to tighten the lace